

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS ✓
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Problem Image Mailbox.**

Fig. 1

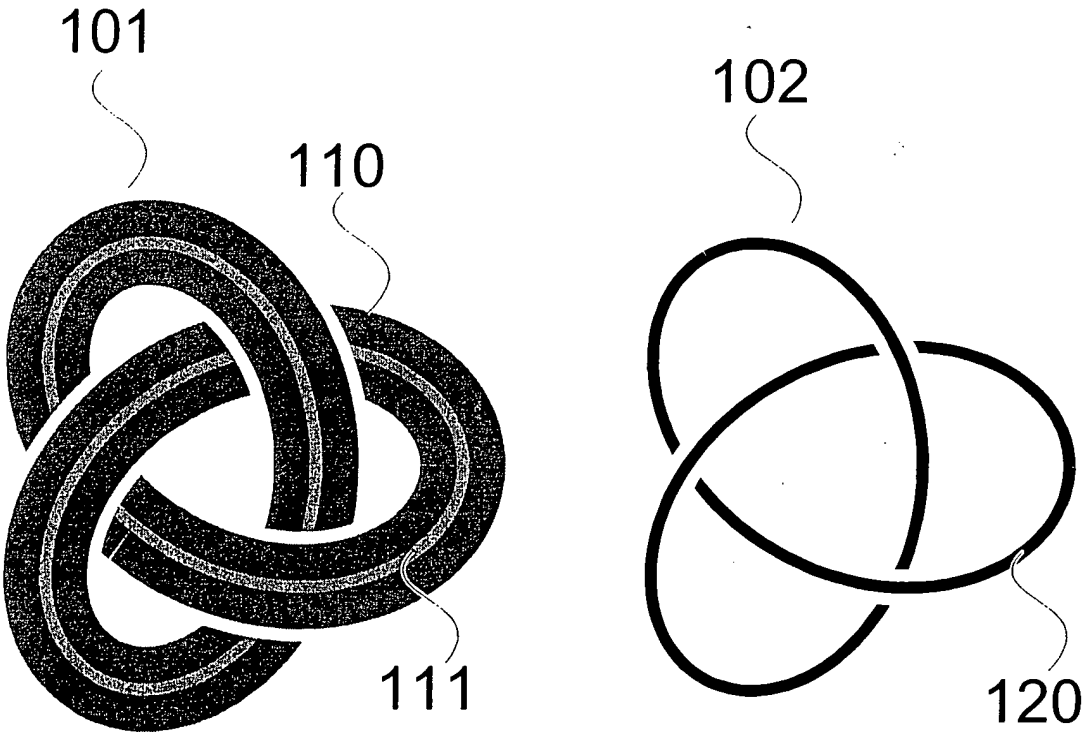


Fig. 2

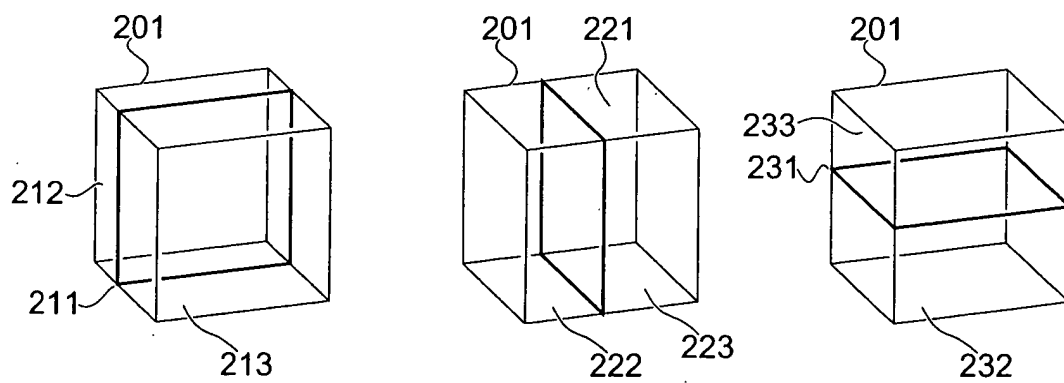


Fig. 3a

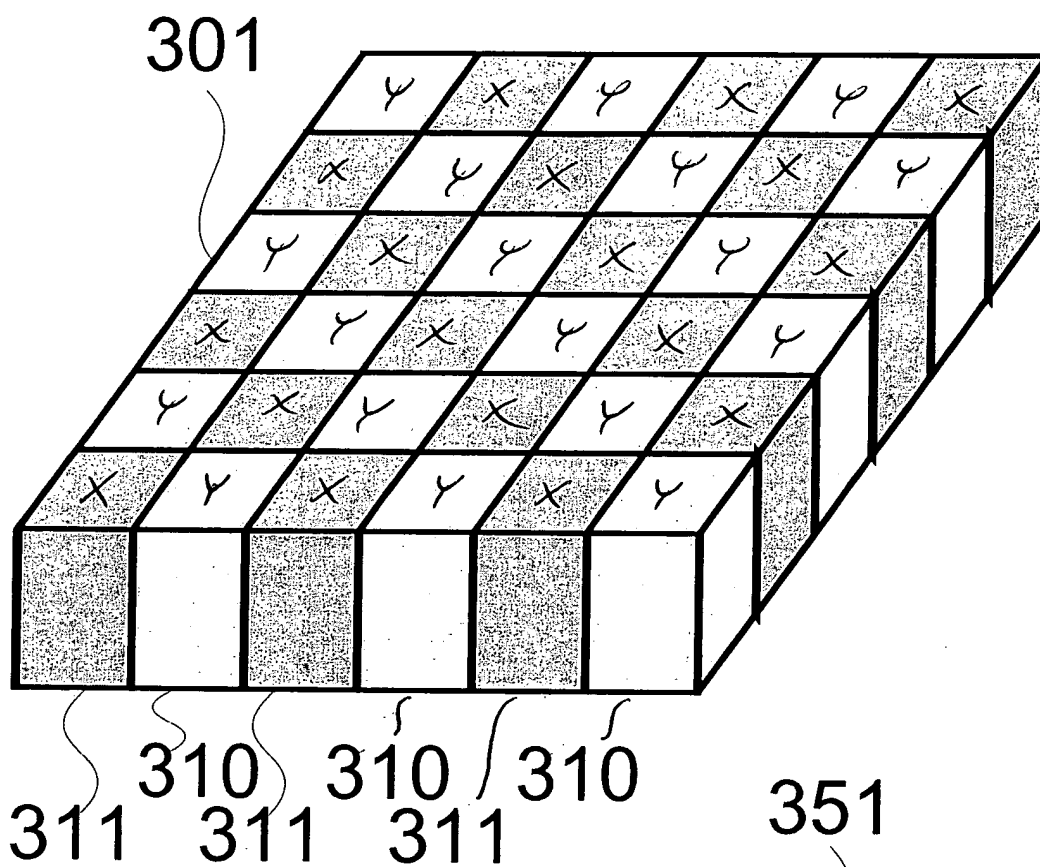


Fig. 3b

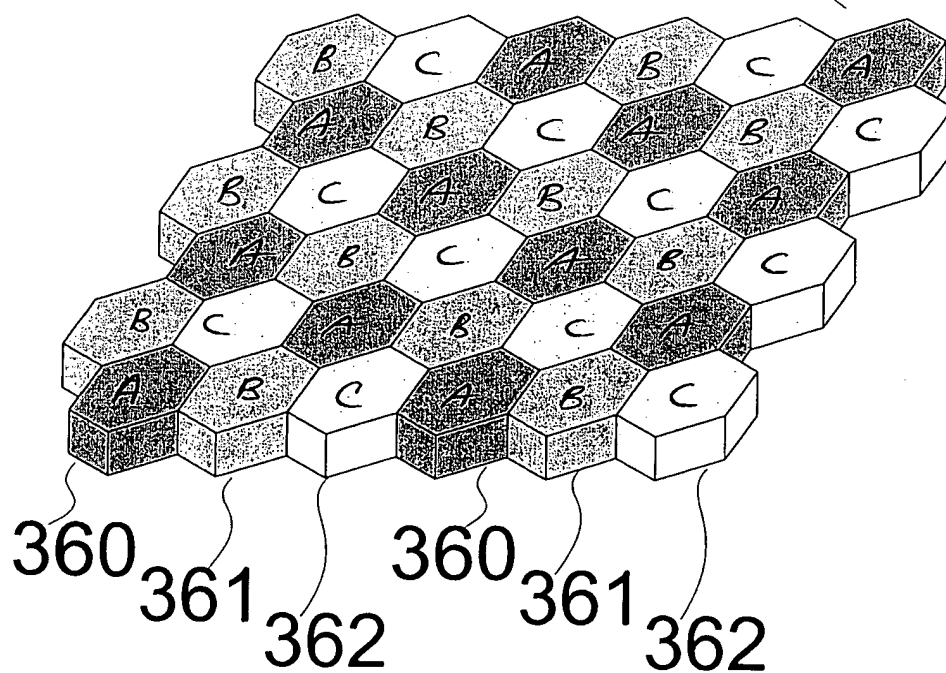


Fig. 4

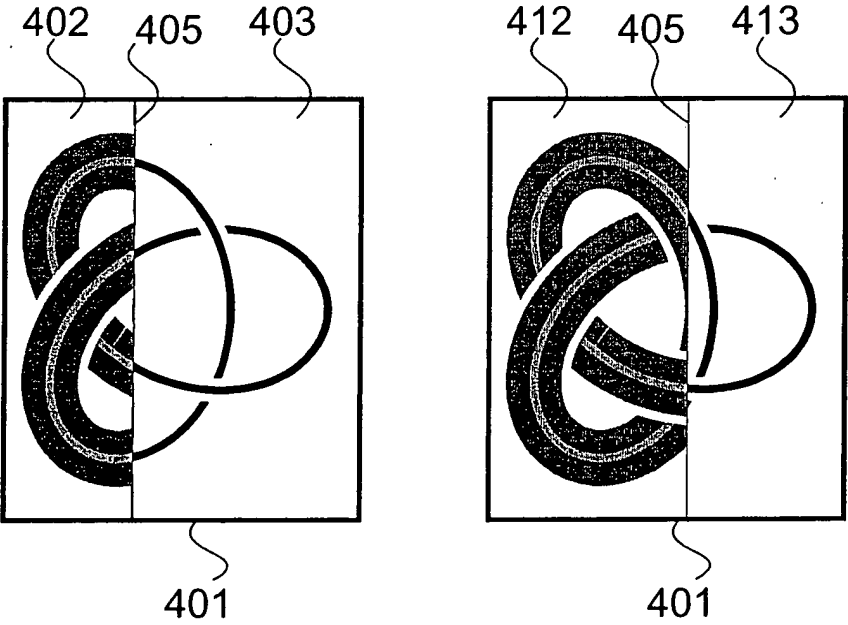


Fig. 5

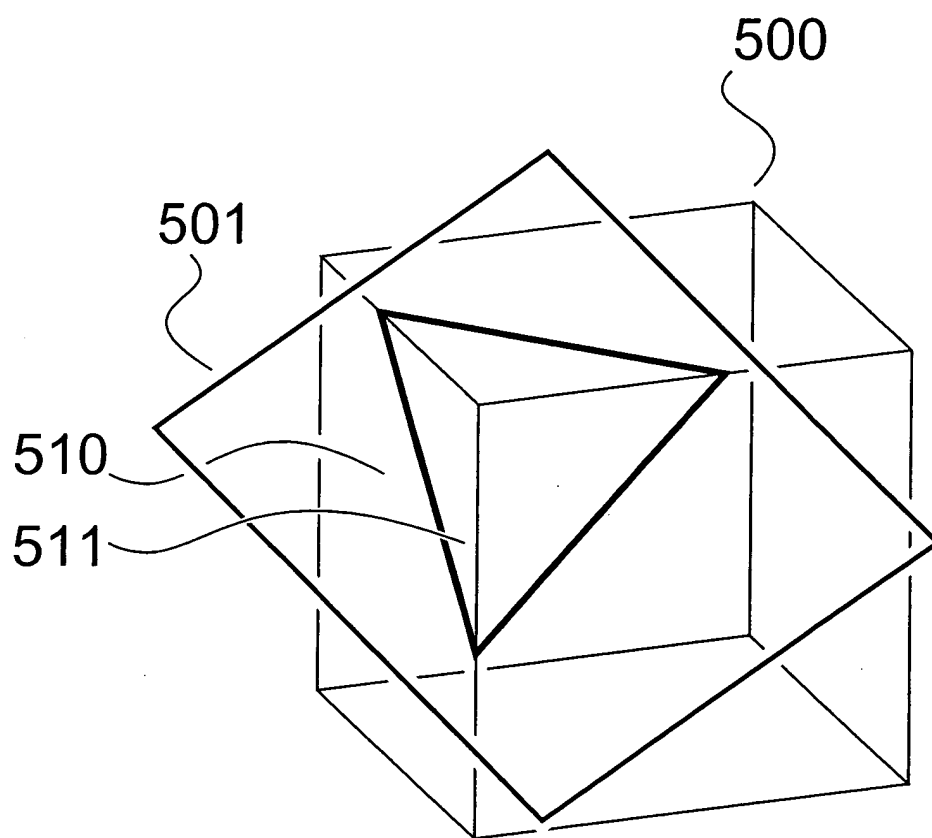


Fig. 6

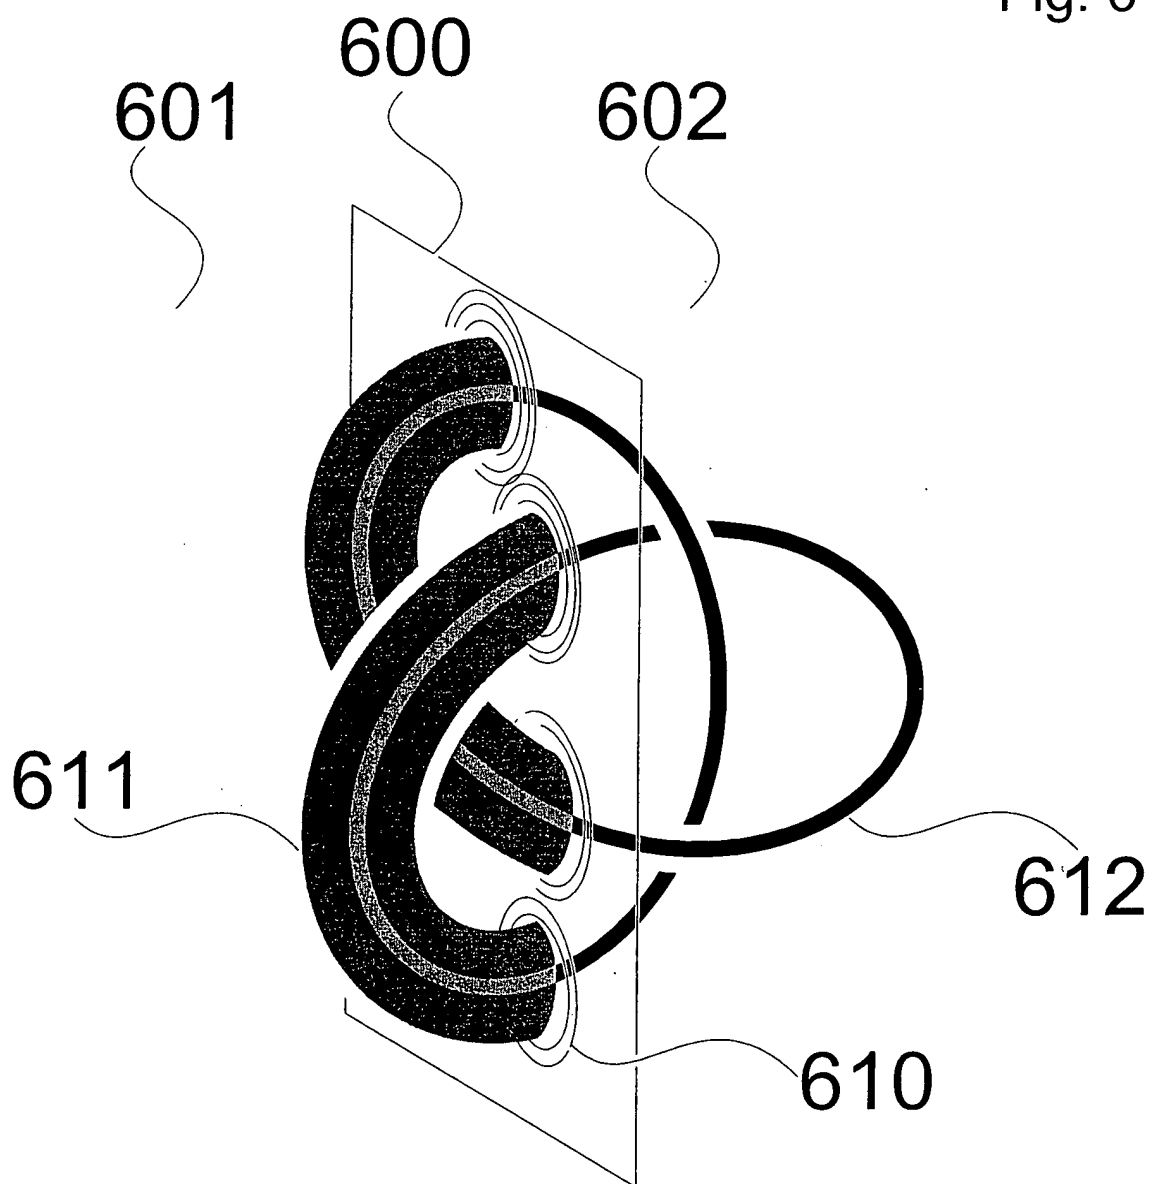


Fig. 7


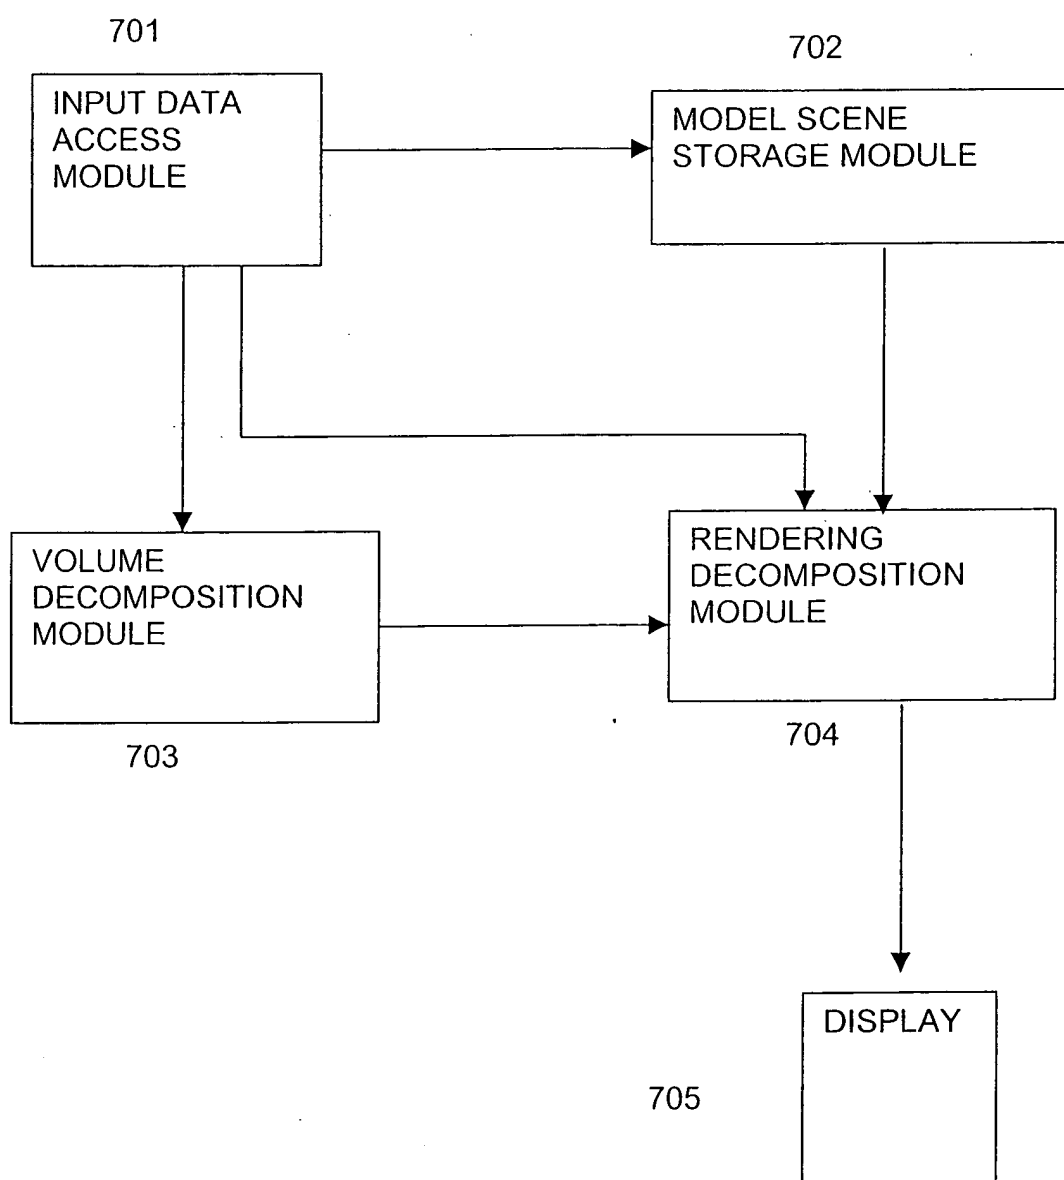




FIG. 8

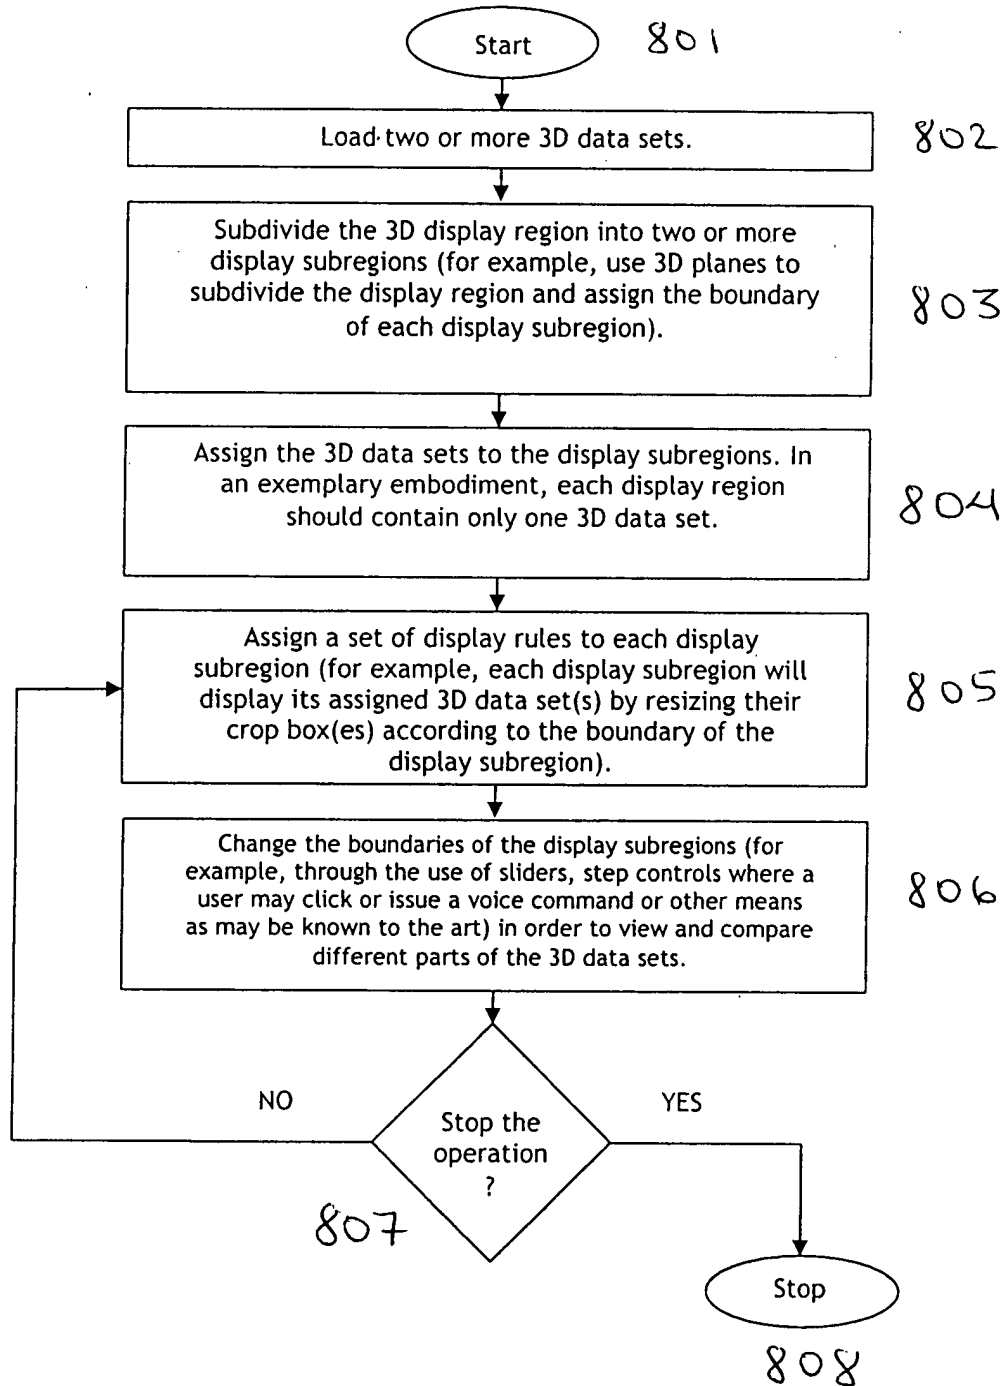

ked object: MRI  
dality:  
ie:  
ie:  
e: 256x256x52, 3.3MB

120  
100  
80  
60  
40  
20  
0

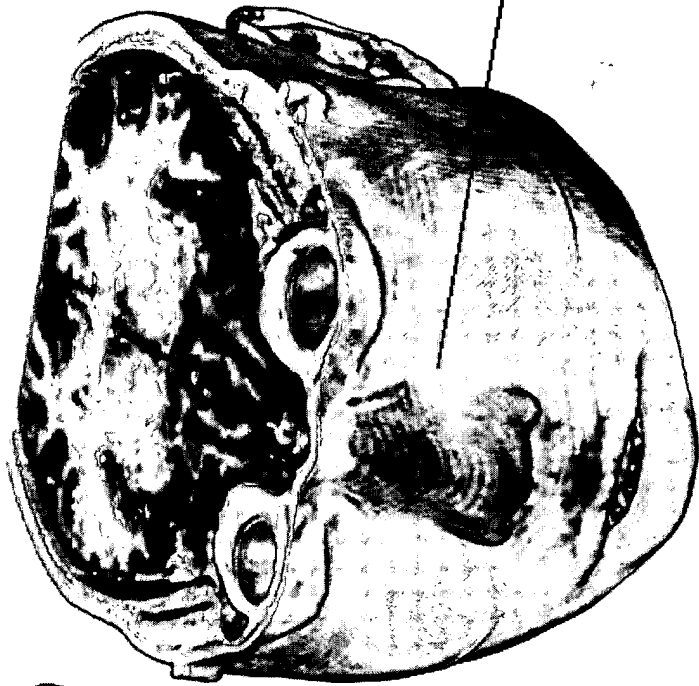
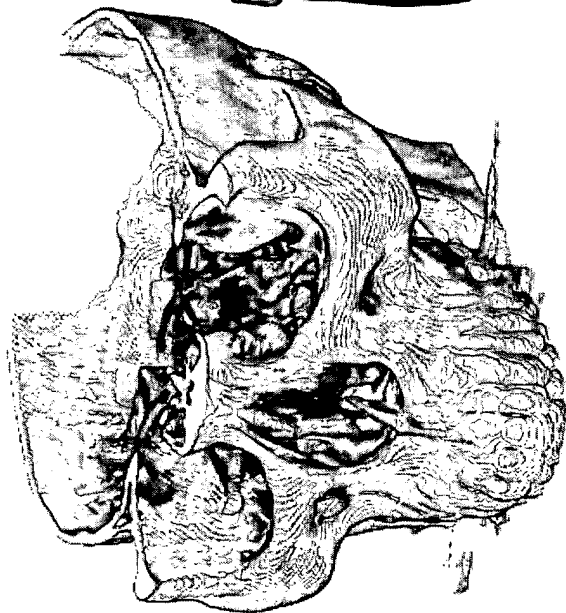


Fig. 9

# Automatic Registrati

ected object: MRI  
dality:  
e:  
e: 256x256x52, 3.3MB


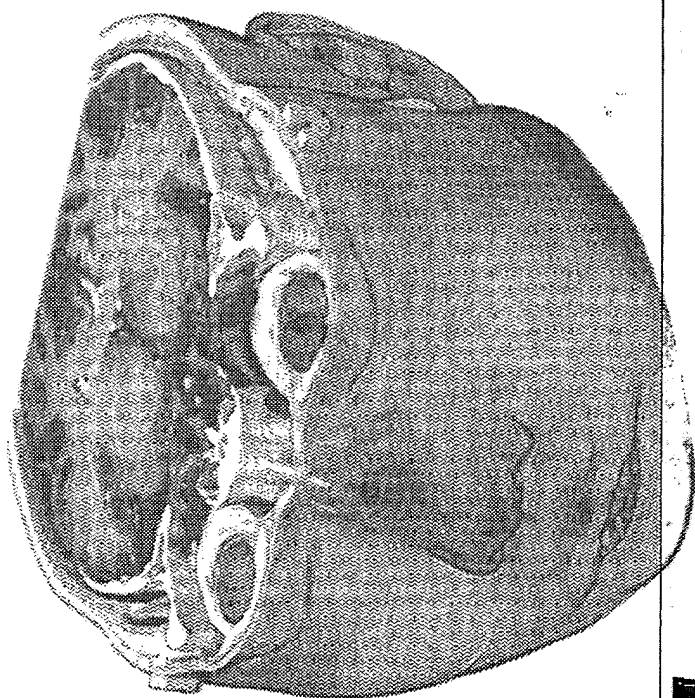


Fig. 10

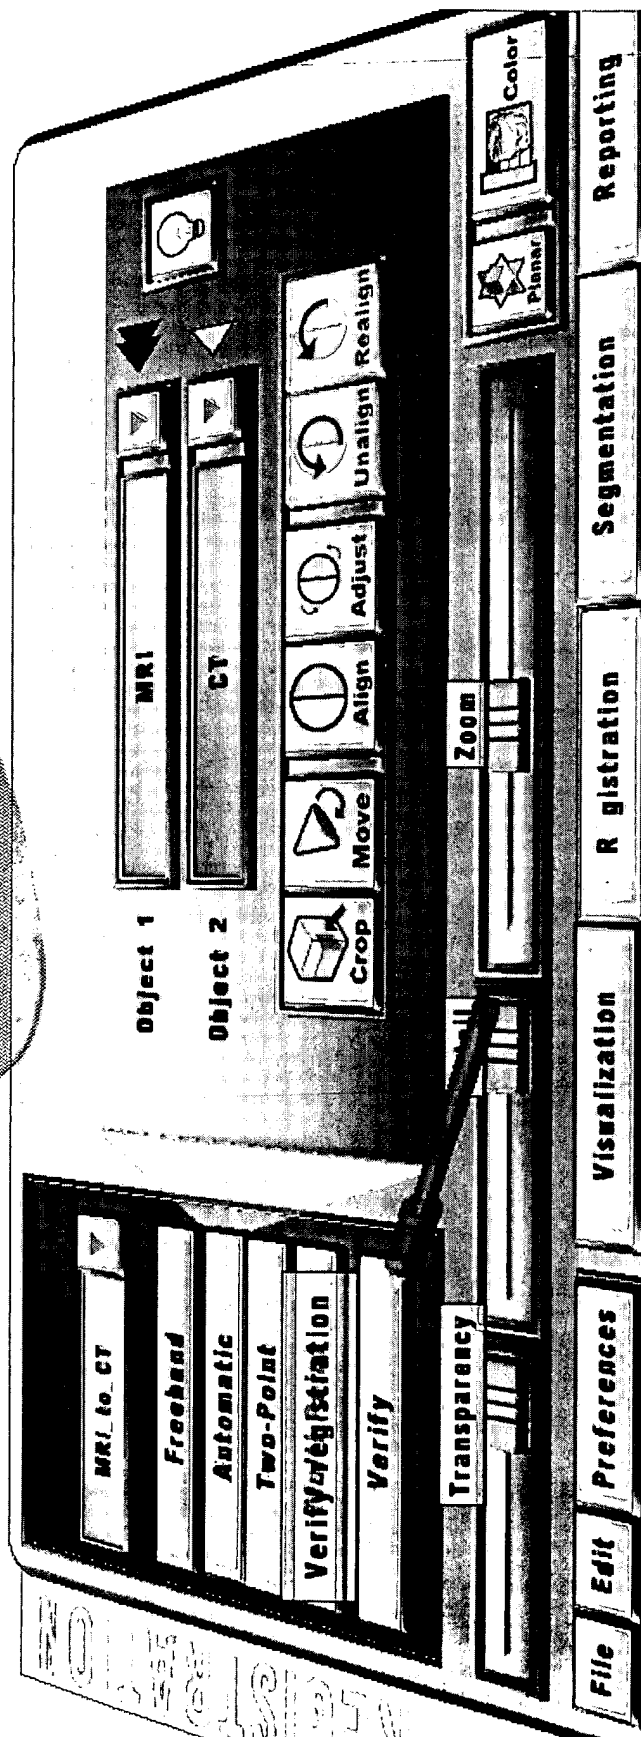

# Verify Registrati

ected object: MRI  
dality:  
e:  
e:  
e: 256x256x52, 3.3MB


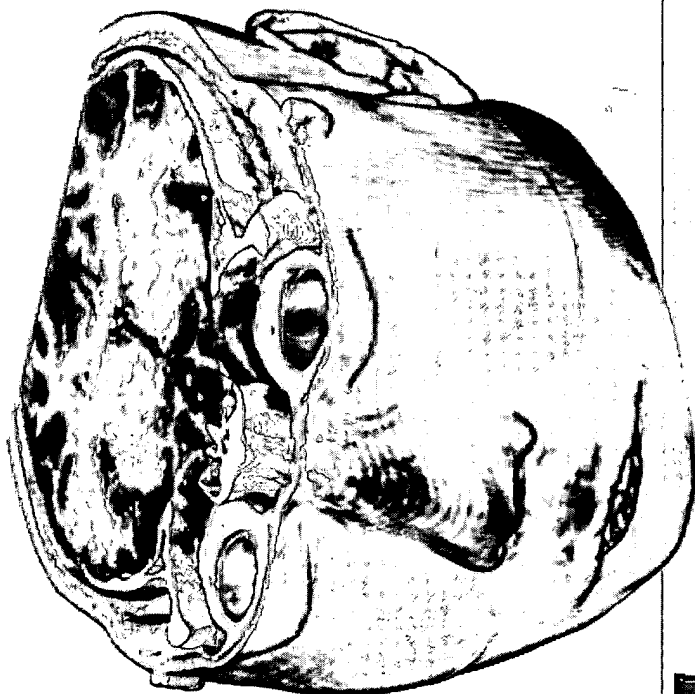


Fig. 11

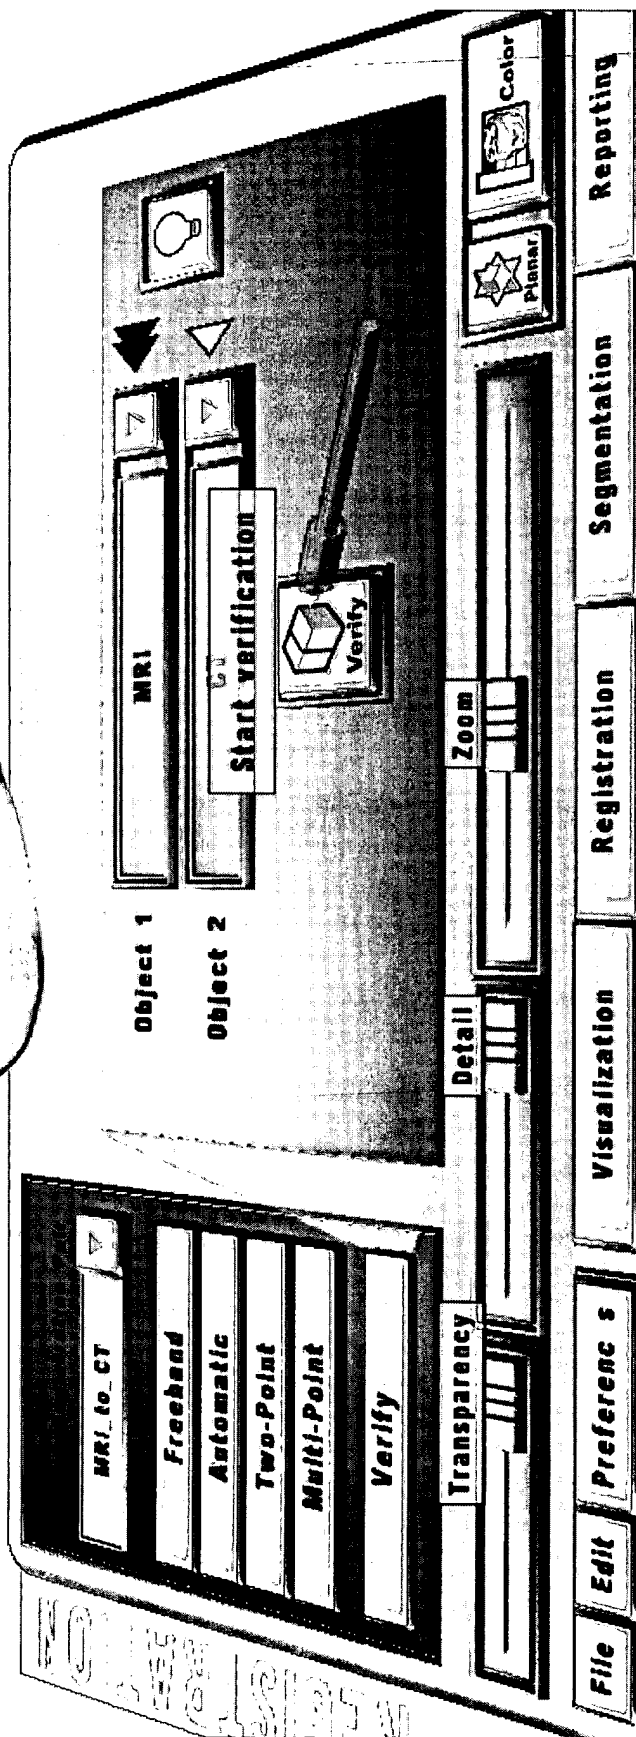

# Verify Registrati

ected object: MRI  
dality:  
e:  
ie:  
e: 256x256x52, 3.3MB

Fig. 12






## Verify Registrati

**ected object: MRI**

**dality:**

161

**B: 256x256x52, 3.3MB**

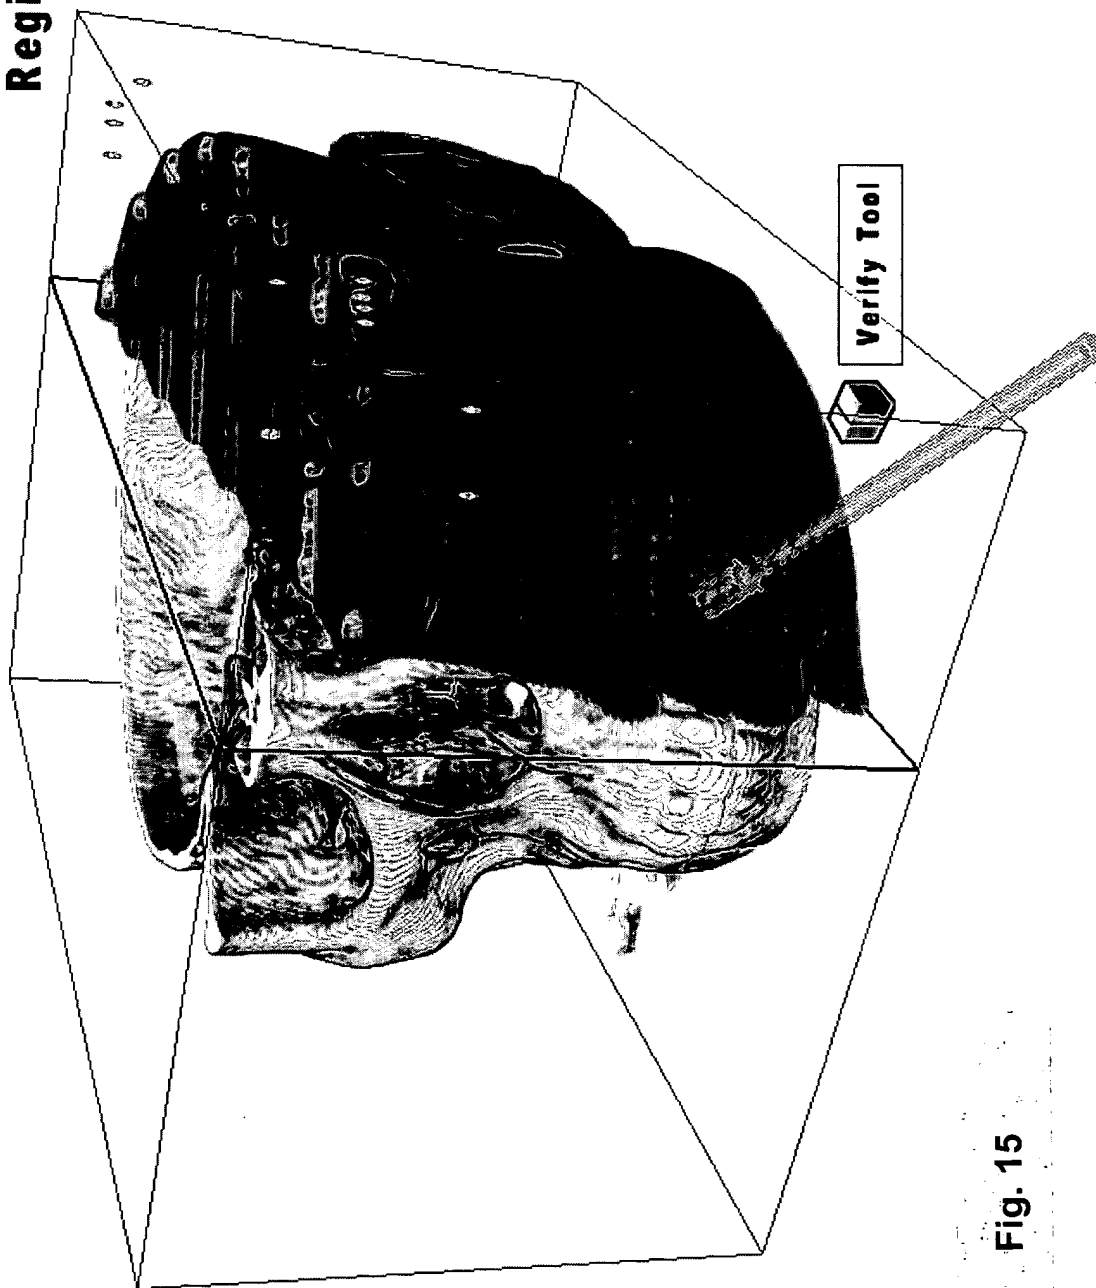

**Fig. 15**

ected object: MRI

ality:

ie:

ie:

e: 256x256x52, 3.3MB

144  
100  
88  
80  
78  
60  
58  
48  
38  
28  
10  
0

# Verify Registrati

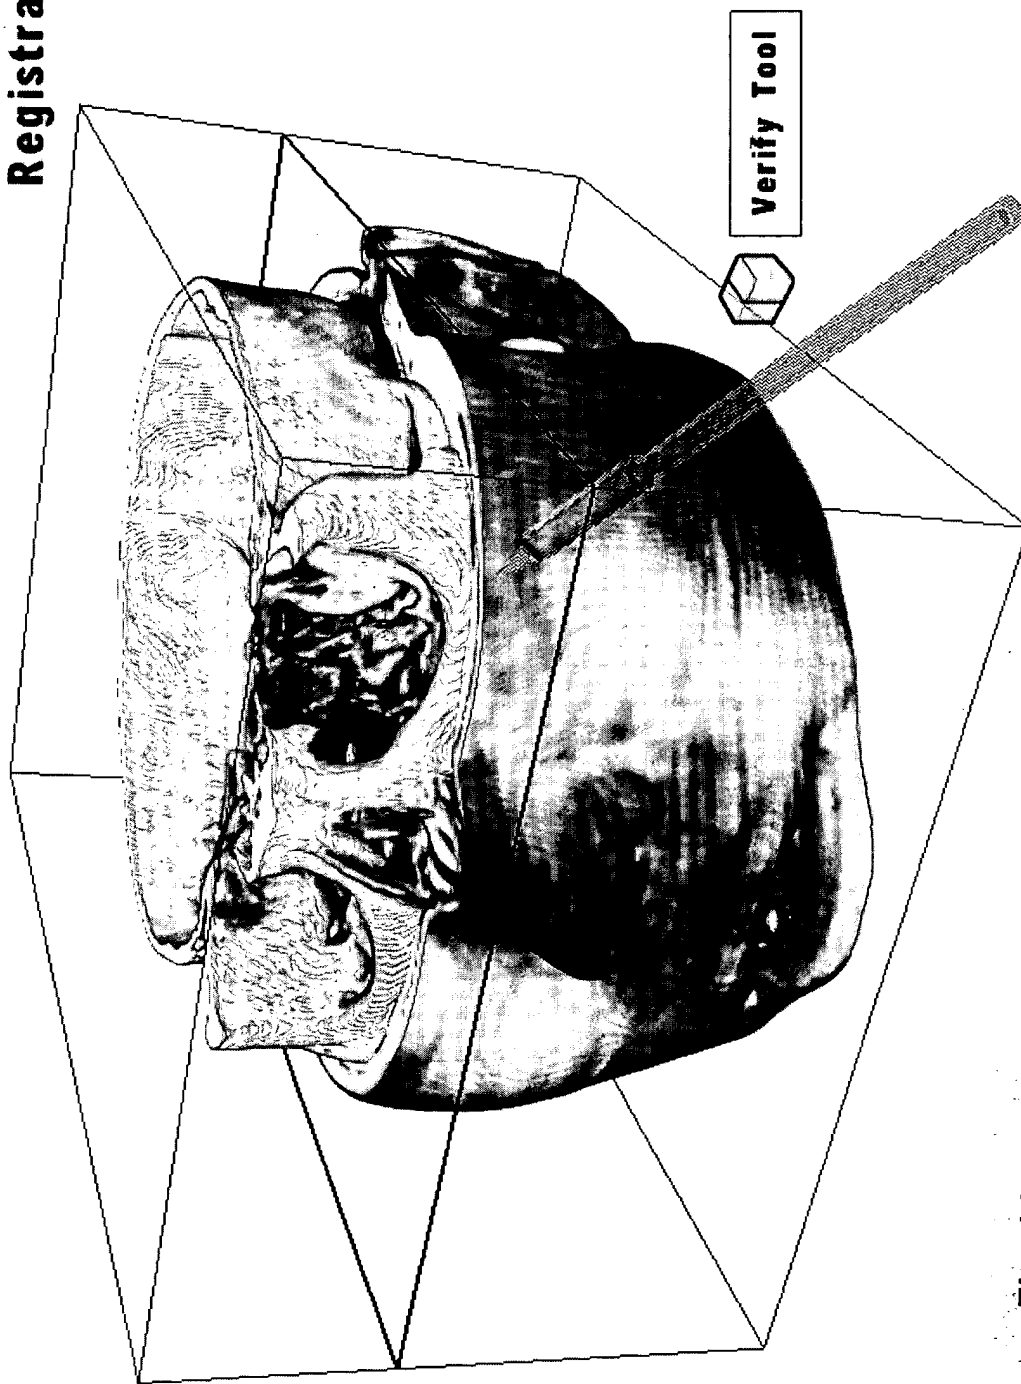


Fig. 14



ected object: MRI

dality:

ie:

ie:

e: 256x256x52, 3.3MB

# Verify Registrati

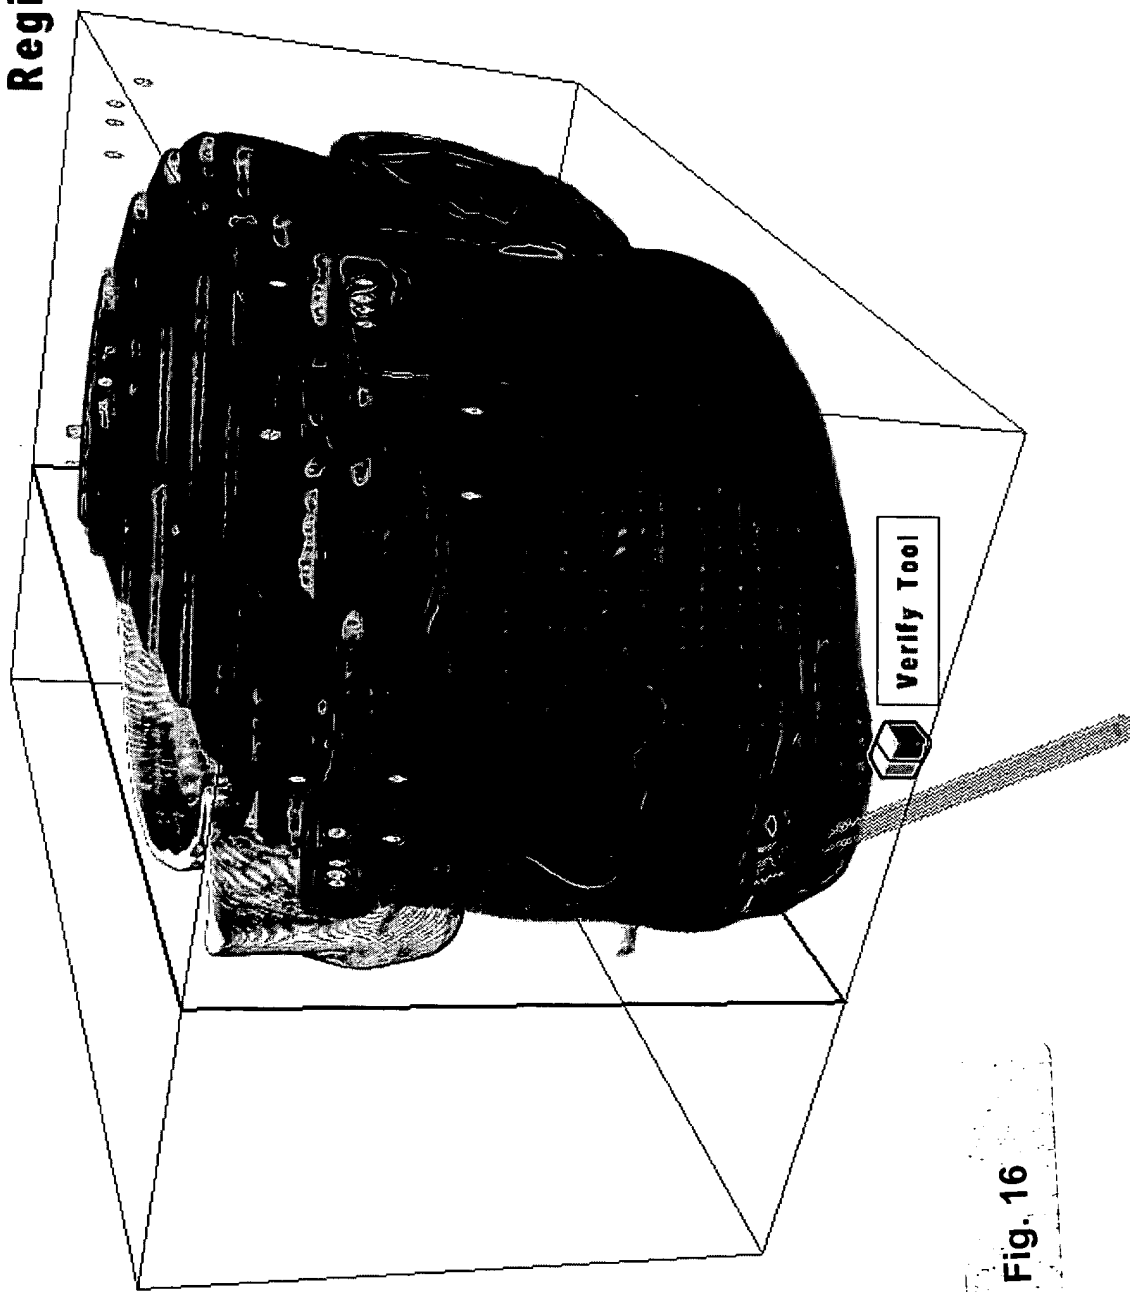


Fig. 16

199  
120  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31


ected object: MRI  
 dality:  
 ie:  
 ie:  
 e: 256x256x52, 3.3MB

100  
 100  
 140  
 100  
 100  
 20  
 00  
 40  
 20  
 0

Fig. 17




# Verify Registrati

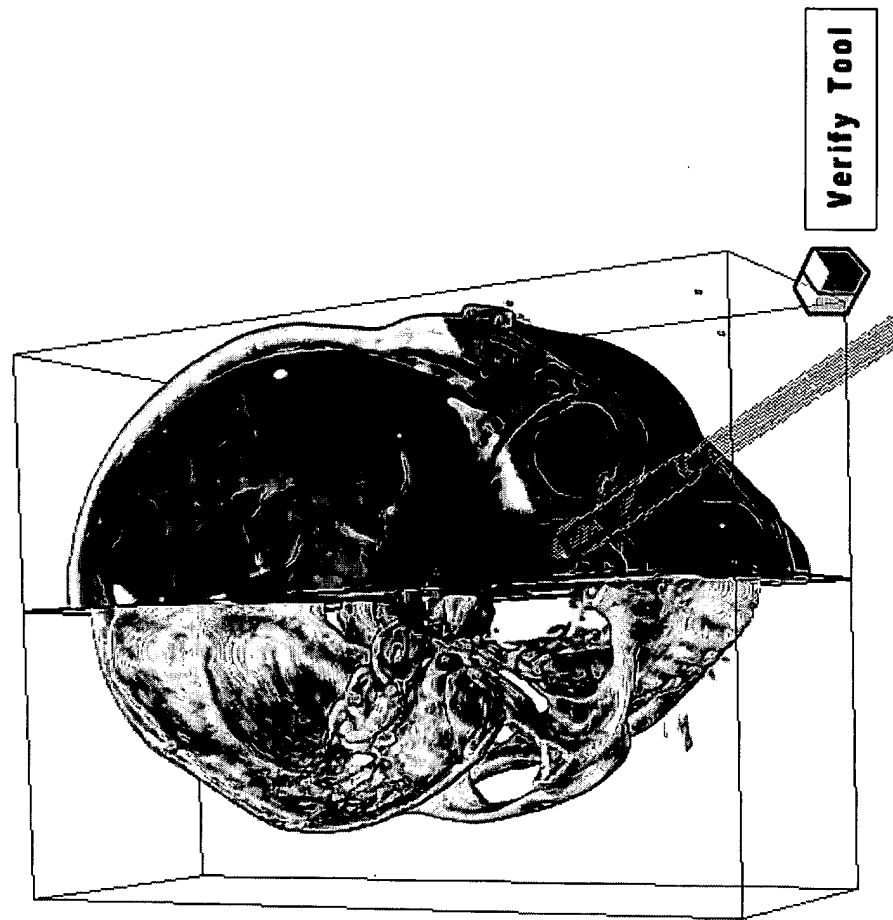

ected object: MRI  
dality:  
ie:  
ie:  
e: 256x256x52, 3.3MB

Verify  
Registrati

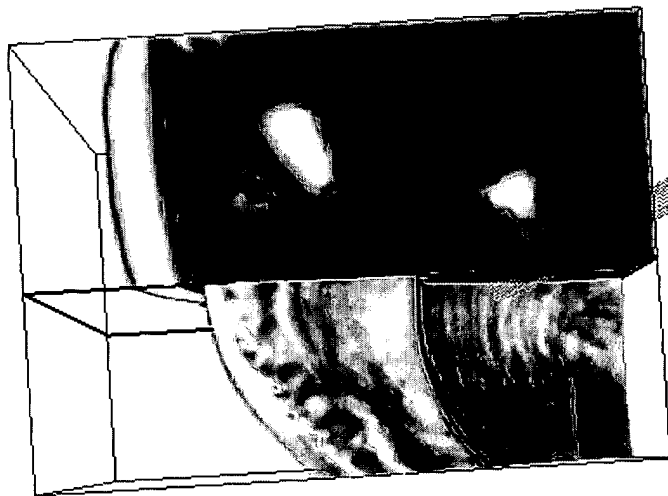

Verify Tool

Fig. 18

ected object: CT  
dality:  
e:  
e: 256x256x75, 4.7MB

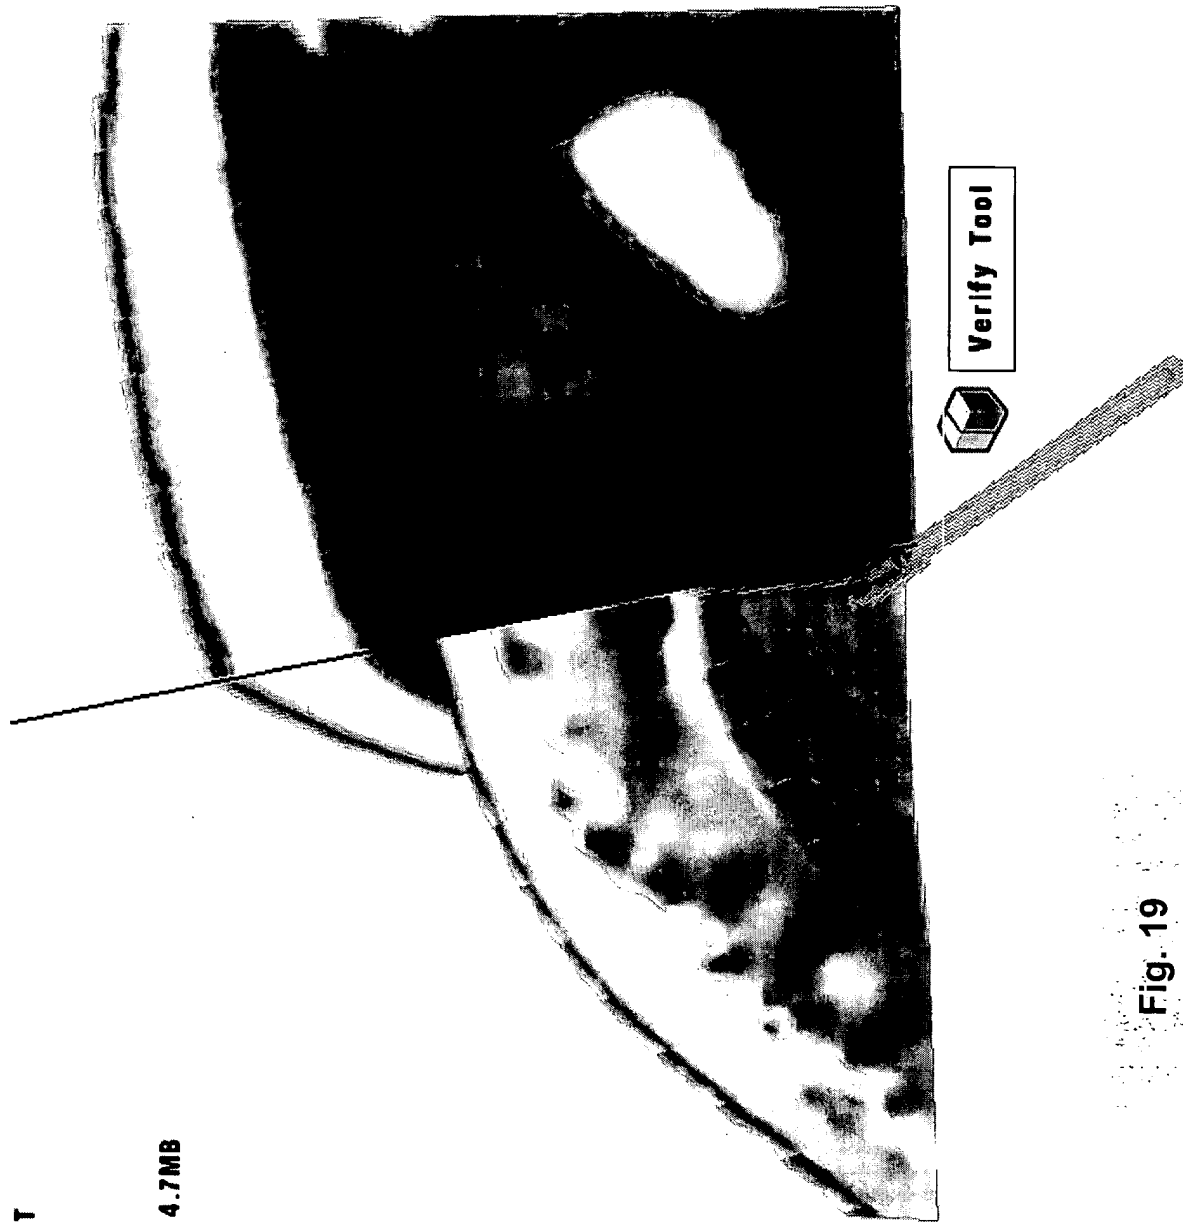


Fig. 19

ected object: CT

dality:

ie:

ie:

e: 256x256x75, 4.7MB

# Verify Registrati



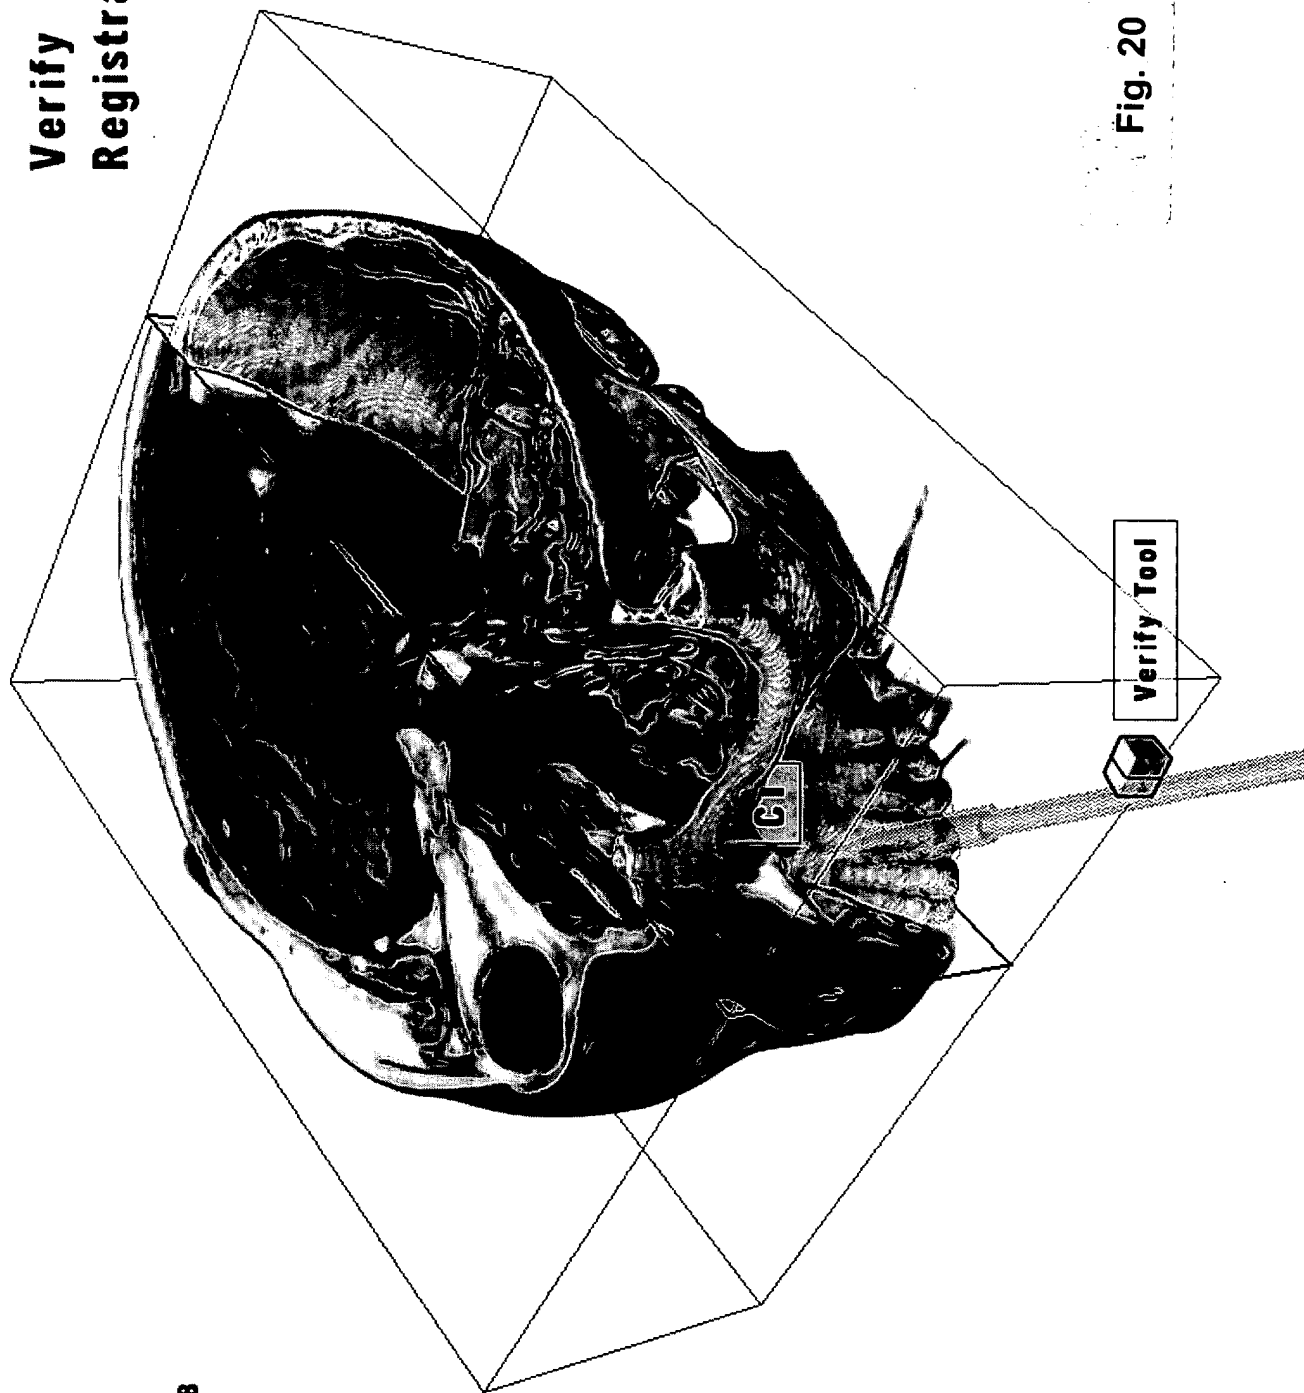


Fig. 20

ected object: CT  
 dality:  
 ie:  
 ie:  
 e: 256x256x75, 4.7MB

100  
 20  
 20  
 70  
 00  
 20  
 40  
 30  
 20  
 10  
 0

Fig. 21

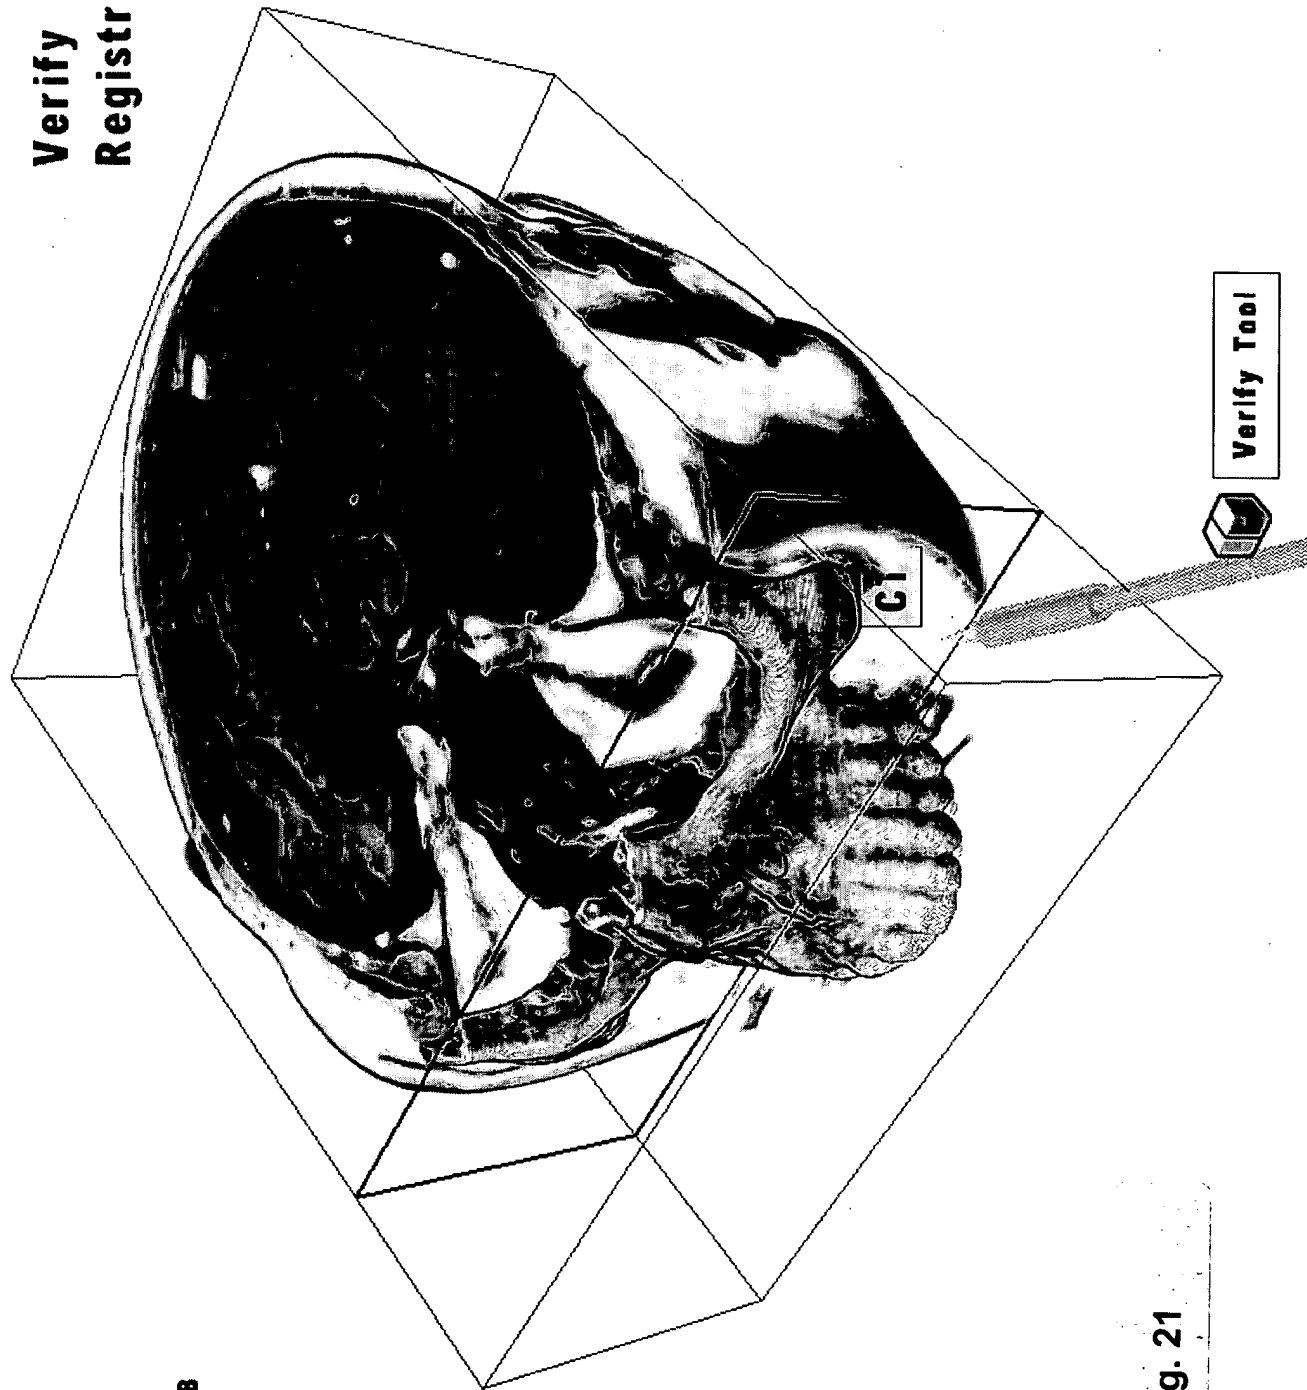

Verify  
 Registrati

Verify Tool

## Verify Registrati

## Verify Tool

**Fig. 22**

ected object: CT  
 dality:  
 e:  
 ie:  
 e: 256x256x75, 4.7MB

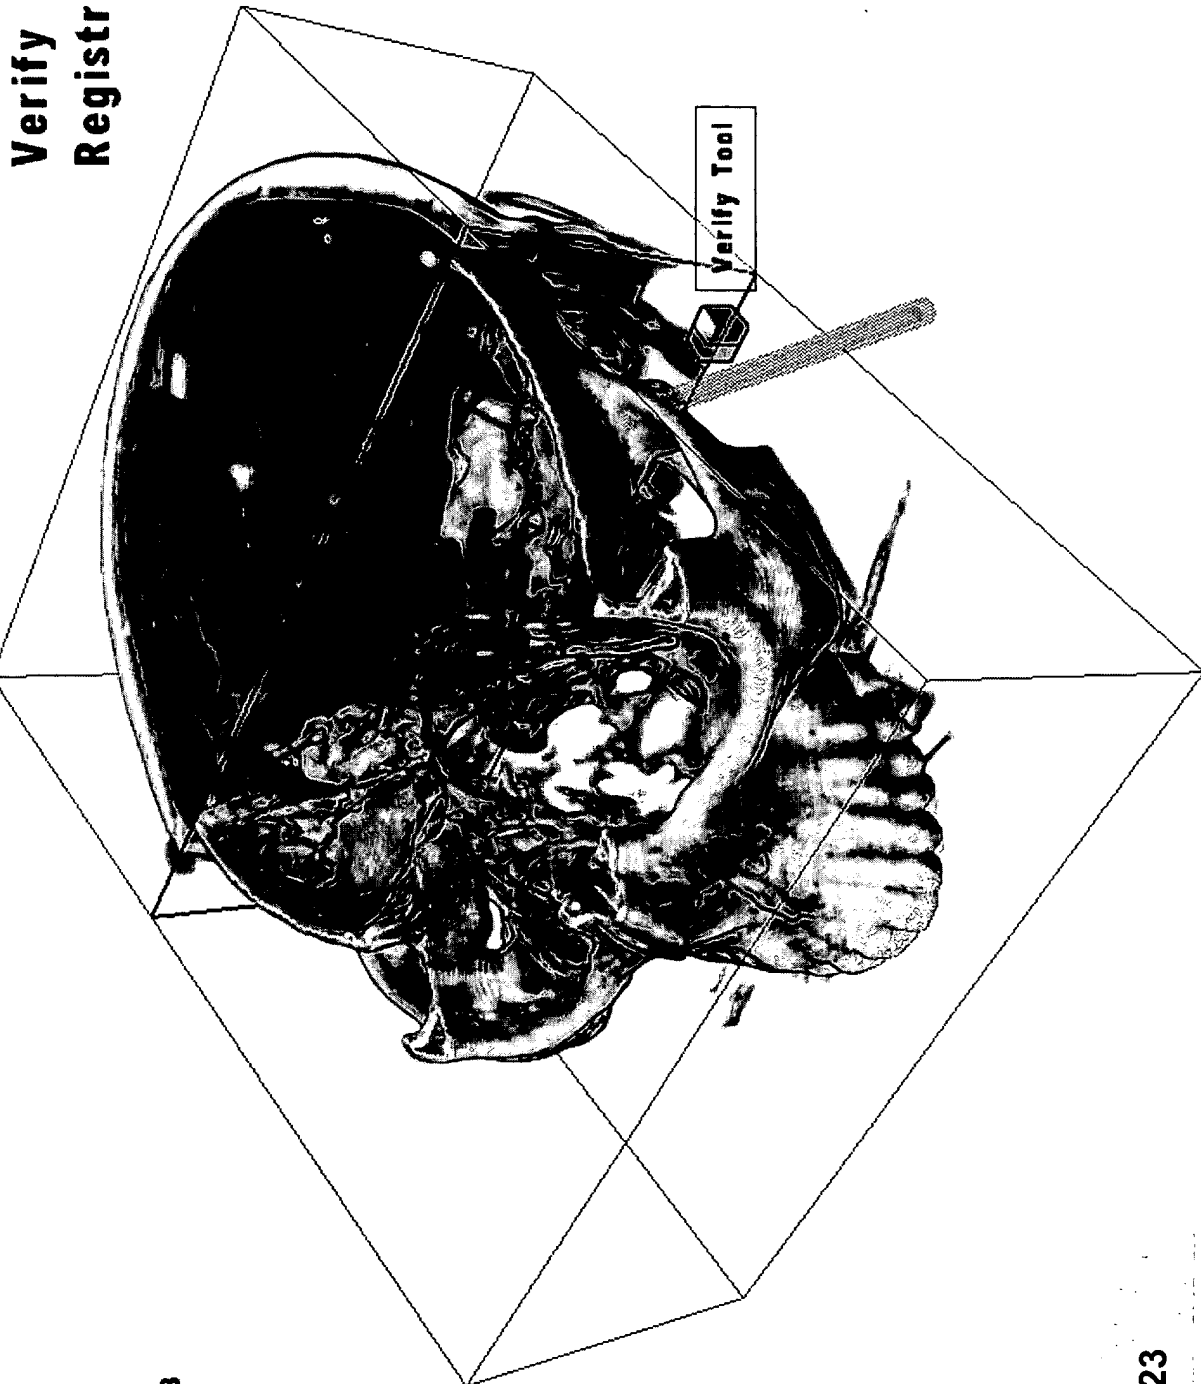


Fig. 23



ected object: CT

dality:

ie:

ie:

e: 256x256x75, 4.7MB

# Verify Registrati


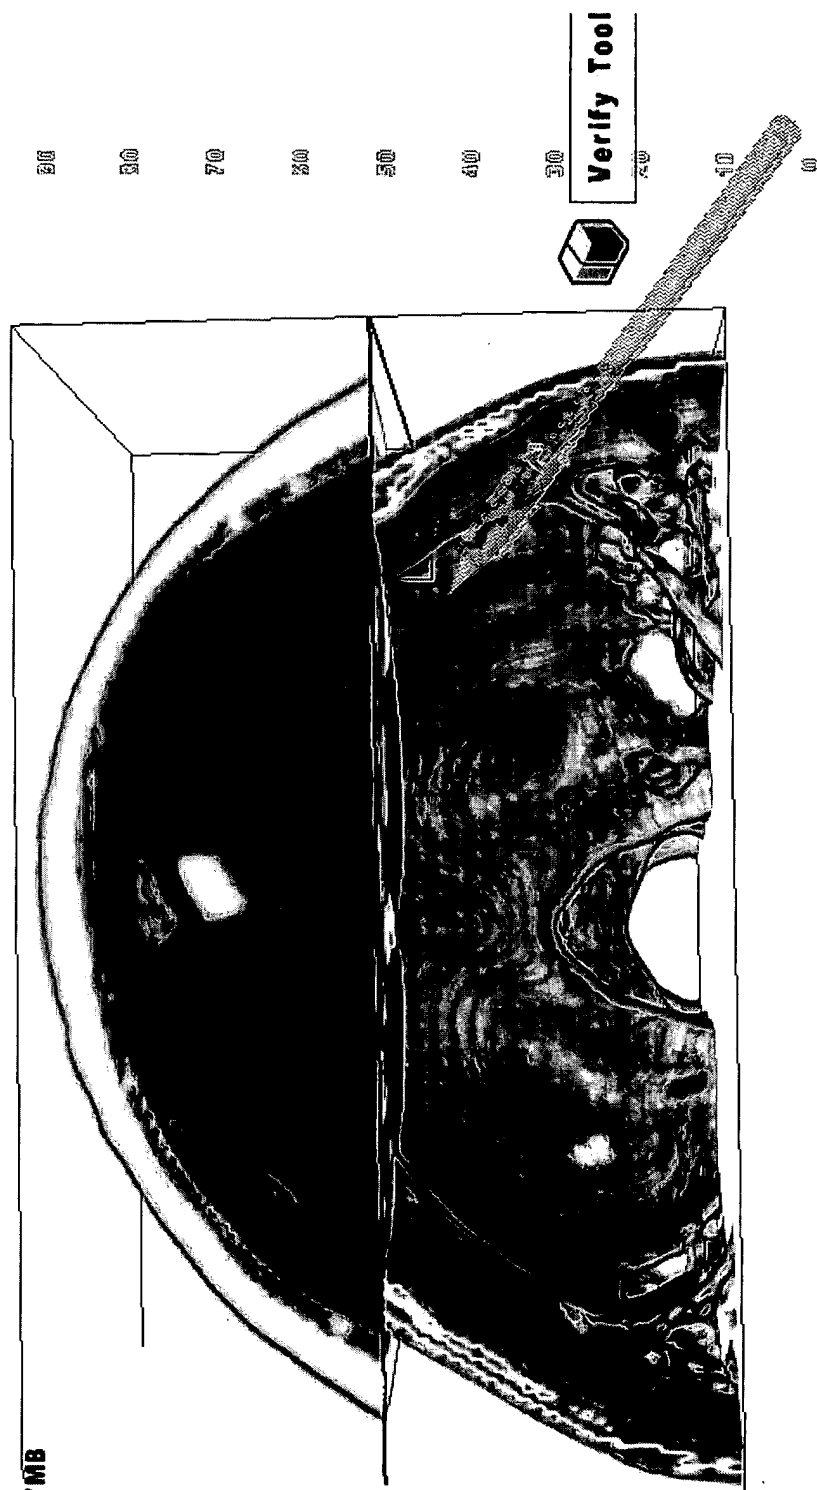


Fig. 24



# Verify Registration

ected object: CT

dality:

ie:

ie:

e: 256x256x75, 4.7MB

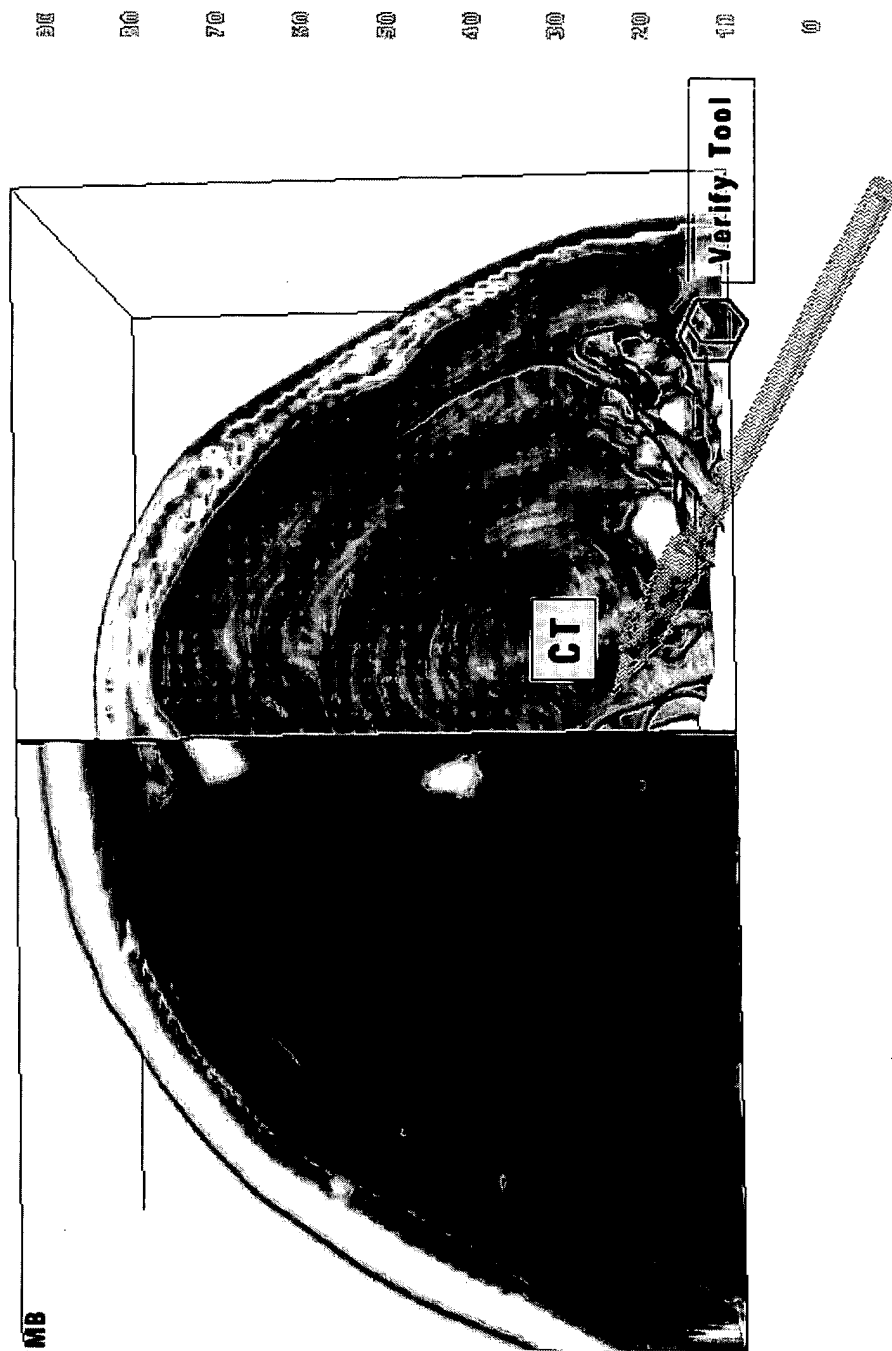


Fig. 25


ected object: CT

dality:

ie:

ie:


e: 256x256x75, 4.7MB



# Verify Registrati



Verify Tool



300  
30  
70  
300  
50  
40  
30  
20  
10  
0

Fig. 26

ected object: CT  
dality:  
e:  
e:  
e: 256x256x75, 4.7MB



# Verify Registrati

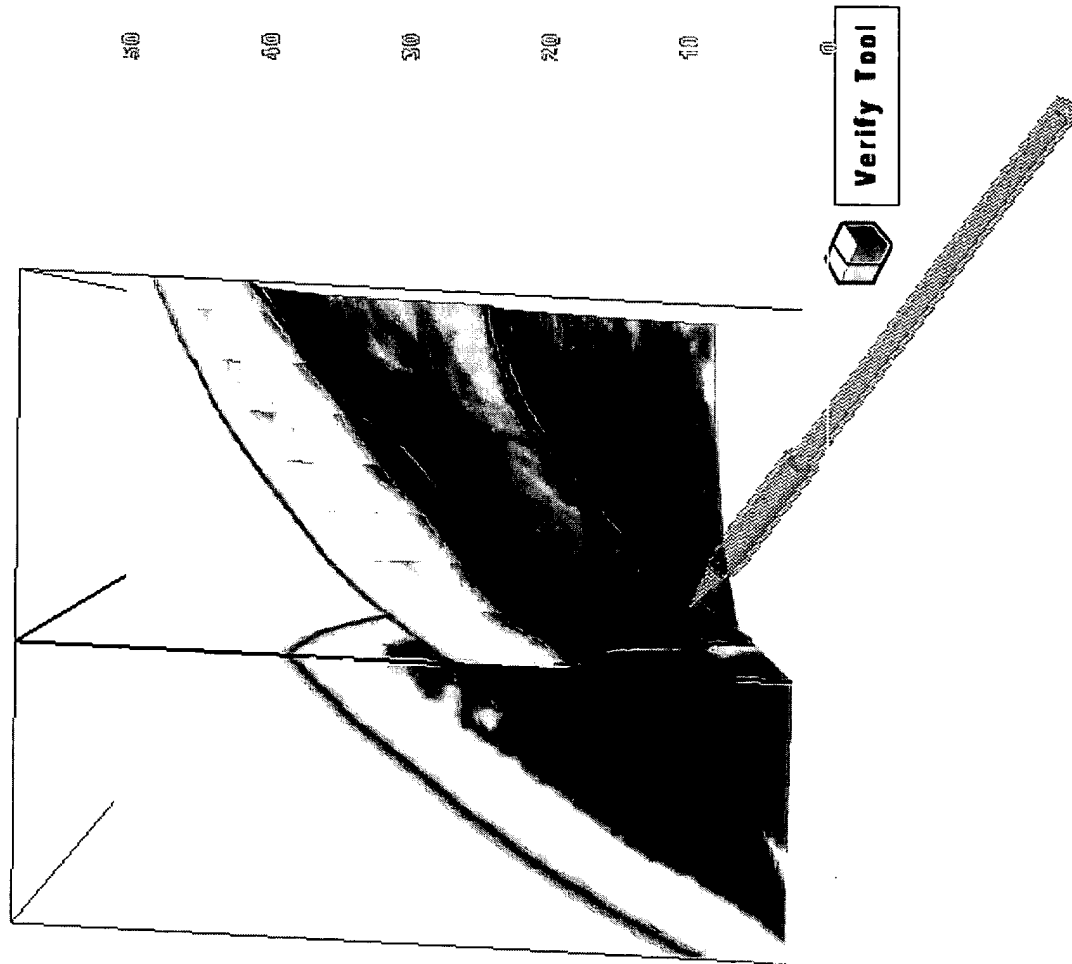


Fig. 27

ected object: CT

dality:

ie:

ie:

e: 256x256x75, 4.7MB



800

Verify

Registrati

800

800

400

500

700

1000

0

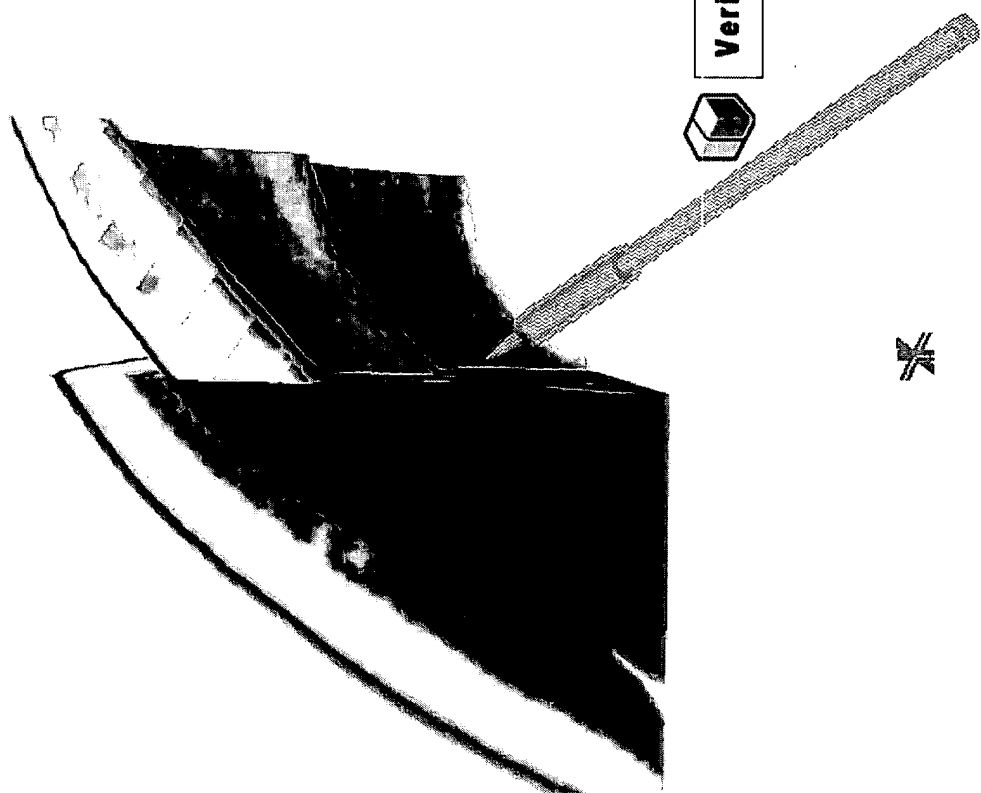


Fig. 28